WARNINGS

- Do not use on animals with implanted electronic medical devices (such as pacemakers or neurostimulators) in the treatment area.
- Do not use on pregnant animals.
- Device is non-sterile. When treating an open wound, place sterile gauze between the device and the wound.
- Do not allow the device to bear weight or become crushed.
- Discontinue use if skin irritation develops.
- If symptoms worsen or fail to improve, consult your veterinarian.

QUESTIONS, COMMENTS, CONCERNS:
CALL 1-301-874-4890 MONDAY-FRIDAY
9AM-4PM

BioElectronics

Manufactured by: BioElectronics Corporation
3880 Roundtree Road, Unit 1 | Jefferson, MD 21755 USA
www.bielcorp.com | 1-301-874-4890 | Stock Symbol: BIEL

U.S. PATENT #7551957B2, U.S PATENT #8412328, CANADA PATENT #2518210,
AUSTRALIA PATENT #2014201303, EUROPEAN PATENT #1606010,
CHINA PATENT #ZL2011200863544, & U.S. AND FOREIGN PATENTS PENDING

LATEX 15% 90% NON STERILE Product is Non-Sterile Attention, see warning statement -13°F 158°F 50 kPa 106 kPa Non-ionizing Radiation Type BF Applied Part

Read instructions before using

DFU-VET-ENG-102
08-04-2026



BENEFITS

- **Drug-Free Pain Relief**
- **Wearable Continuous Therapy**
- **Helps Reduce Pain and Inflammation**
- **Supports Improved Mobility**
- **Comfortable for Daily Wear**
- **For Dogs, Cats & Horses**

WARNINGS

- Do not use on animals with implanted electronic medical devices (such as pacemakers or neurostimulators) in the treatment area.
- Do not use on pregnant animals.
- Device is non-sterile. When treating an open wound, place sterile gauze between the device and the wound.
- Do not allow the device to bear weight or become crushed.
- Discontinue use if skin irritation develops.
- If symptoms worsen or fail to improve, consult your veterinarian.

QUESTIONS, COMMENTS, CONCERNS:
CALL 1-301-874-4890 MONDAY-FRIDAY
9AM-4PM

BioElectronics

Manufactured by: BioElectronics Corporation
3880 Roundtree Road, Unit 1 | Jefferson, MD 21755 USA
www.bielcorp.com | 1-301-874-4890 | Stock Symbol: BIEL

U.S. PATENT #7551957B2, U.S PATENT #8412328, CANADA PATENT #2518210,
AUSTRALIA PATENT #2014201303, EUROPEAN PATENT #1606010,
CHINA PATENT #ZL2011200863544, & U.S. AND FOREIGN PATENTS PENDING

LATEX 15% 90% NON STERILE Product is Non-Sterile Attention, see warning statement -13°F 158°F 50 kPa 106 kPa Non-ionizing Radiation Type BF Applied Part

Read instructions before using

DFU-VET-ENG-102
08-04-2026



BENEFITS


- **Drug-Free Pain Relief**
- **Wearable Continuous Therapy**
- **Helps Reduce Pain and Inflammation**
- **Supports Improved Mobility**
- **Comfortable for Daily Wear**
- **For Dogs, Cats & Horses**


DEVICE ACTIVATION

HOW TO TURN THE DEVICE ON:
Step 1: To activate the device, remove the white tab from the back of the device and push the silver on/off button for 1-2 seconds. Release the button.


Step 2: Once the device is activated, the green LED light on the front of the device will turn on. If the green LED light does not turn on, please repeat Step 1.

HOW TO TURN THE DEVICE OFF:
To deactivate the device, press the silver button and hold it down for 1-2 seconds. Once the device is deactivated, the green LED light will turn off.







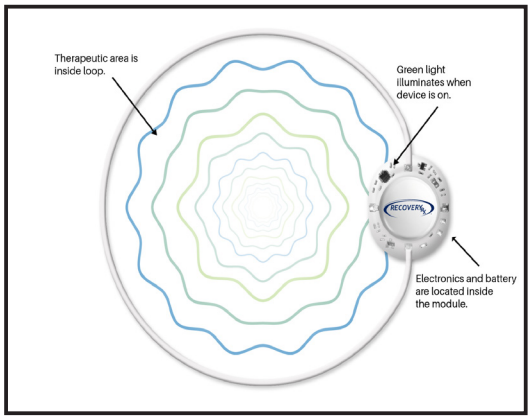


FOR CLINICAL INFORMATION VISIT:
http://recoveryrxvet.com


4 STEPS TO PAIN RELIEF FOR ANIMALS

1. Turn on the device by pushing the silver button on the Loop. (SEE INSTRUCTIONS FOR DEVICE ACTIVATION)
2. Place on the animal's collar at the cervical spine OR over the area of injury.
3. To attach to legs of a horse use cohesive bandages such as VetWrap to secure. Do not over-tighten as this may restrict circulation.
4. Do not let unit get wet. If you expect the animal to get wet either in rain or rolling in wet grass or snow place the device in a Ziploc bag or wrap in a plastic sheet before placing the device over the injury. Similarly if you expect the wound to ooze or discharge a significant amount of pus, place the unit in a Ziploc bag before putting over a sterile dressing on the wound.

FOR BEST RESULTS:
For best results, use continuously whenever possible. RecoveryRx Vet may be worn up to 24 hours per day throughout the 720-hour treatment period.









DEVICE ACTIVATION

HOW TO TURN THE DEVICE ON:
Step 1: To activate the device, remove the white tab from the back of the device and push the silver on/off button for 1-2 seconds. Release the button.


Step 2: Once the device is activated, the green LED light on the front of the device will turn on. If the green LED light does not turn on, please repeat Step 1.

HOW TO TURN THE DEVICE OFF:
To deactivate the device, press the silver button and hold it down for 1-2 seconds. Once the device is deactivated, the green LED light will turn off.







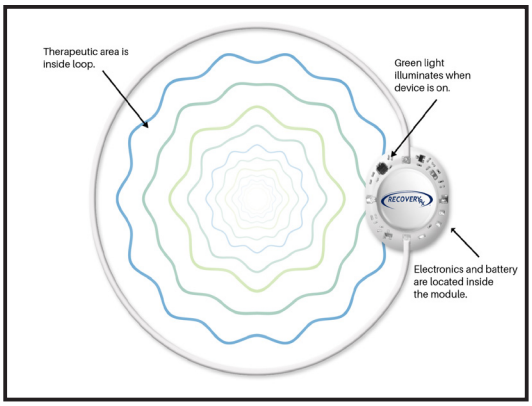

FOR CLINICAL INFORMATION VISIT:
http://recoveryrxvet.com

4 STEPS TO PAIN RELIEF

1. Turn on the device by pushing the silver button on the Loop. (SEE INSTRUCTIONS FOR DEVICE ACTIVATION)
2. Place on the animal's collar at the cervical spine OR over the area of injury.
3. To attach to legs of a horse use cohesive bandages such as VetWrap to secure. Do not over-tighten as this may restrict circulation.
4. Do not let unit get wet. If you expect the animal to get wet either in rain or rolling in wet grass or snow place the device in a Ziploc bag or wrap in a plastic sheet before placing the device over the injury. Similarly if you expect the wound to ooze or discharge a significant amount of pus, place the unit in a Ziploc bag before putting over a sterile dressing on the wound.

FOR BEST RESULTS:
For best results, use continuously whenever possible. RecoveryRx Vet may be worn up to 24 hours per day throughout the 720-hour treatment period.

